


ELECTRONIC BLOOD PRESSURE MONITOR

JPD-HA101

Apply the cuff to left upper arm

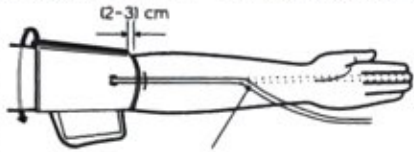


The bottom edge of the cuff should be 2-3cm above the elbow. Air tube is on the inside of your arm and aligned with your middle finger.

Apply the cuff to right upper arm



The air tube will be at the side of your elbow. Be careful not to rest your arm on the air tube.

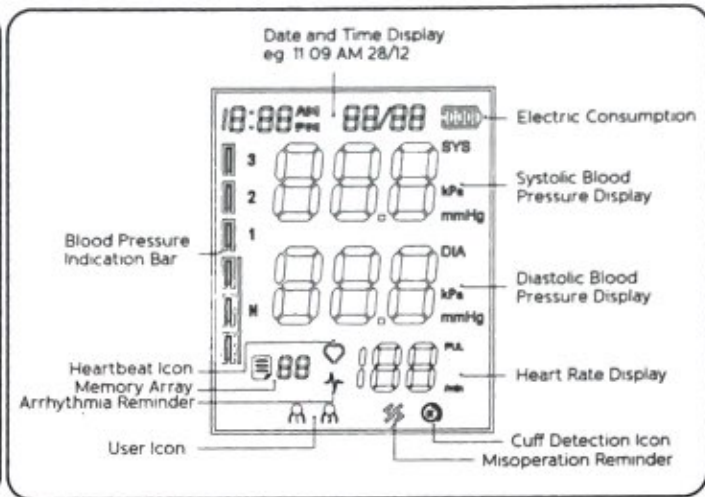

SPECIFICATIONS

Display Mode	Digital display
Measuring Mode	Oscillographic method
Measuring Range	pressure value: 0-295mmHg (0kPa-39.3 kPa) Pulse rate: 40-199 pulse beats/min
Static Measurement Accuracy	Pressure value: ± 0.4 kPa (± 3 mmHg) Pulse rate: $\pm 5\%$ of read value
Memory Storage	99 each for 2 users
Cuff	Upper-arm-type cuff
Accessories	Cuff, User Manual, Zipped Carrying Bag, Dry Battery
Operating environmental conditions	5 °C to 40 °C ; 15% to 85% R.H. ; 70 kPa to 106 kPa
Transport and storage environmental conditions	-20 °C to 55 °C ; 10% to 93% R.H. ; 70 kPa to 106 kPa

EC REP MedPath GmbH
Mies-van-der-Rohe-
Strasse 8, 80807 Munich, Germany

CE 0482



Shenzhen Jumper Medical Equipment Co., Ltd.
D Building, No. 71, Xintian Road, Fuyong Street,
Baoan, Shenzhen, Guangdong, China 518103

Website: www.jumper-medical.com

E-mail: info@jumper-medical.com

Tel: +86-755-26696279 Fax: +86-755-26852025

V2.2
2022.04.19



Made in China